

# Information Data Sheet

**Detector Tube H<sub>2</sub>O-MP(mg/m<sup>3</sup>)**

**Part No. (US): 655791**

**Part No. D5086851**

## 1. Application

Detection of water vapor (H<sub>2</sub>O) in compressed air.

## 2. Sampling Procedure

Monitoring set for compressed air, Uniphos(formerly AUER) Airtester HP, Uniphos (formerly AUER/MSA) Airtester MP, observe included instruction for use.


## 3. Measuring Range

100 mg/ m<sup>3</sup> ... 1000 mg/ m<sup>3</sup> water vapor for a 3 l sample.

## 4. Chemical Reaction and Color Change

Precipitation of selenium from selenium/sulfuric acid by water.

Color change: yellow → brown resp. brown/green.

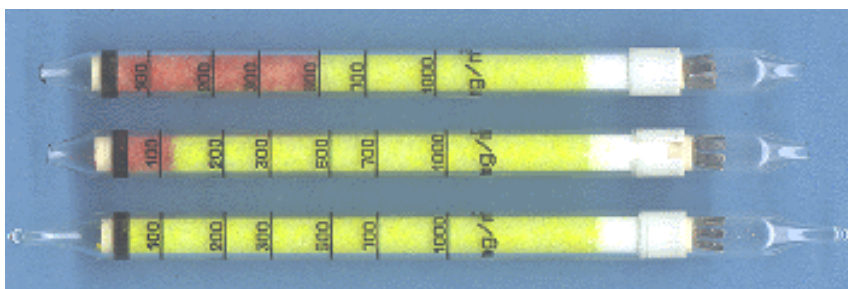

## 5. Influence of Temperature

Detector tubes can be used between 0 °C and 35 °C (32 °F and 95 °F).

The calibration scales on detector tube are exactly valid if tubes have a temperature of 20 °C (68 °F) during measurement. If detector tube temperature deviates from 20 °C (68 °F), multiply reading (mg/ m<sup>3</sup>) with appropriate correction factor (see table)

Temperature of detector tube (°C)	0	5	10	15	20	25	30	35
Temperature of detector tube (°F)	32	41	50	59	68	77	86	95
Correction factor	1,85	1,55	1,35	1,17	1,00	0,85	0,70	0,57

Normally, detector tube temperature is equivalent to ambient temperature.

## 6. Interferences and Cross Sensitivities

No interference from:

– hydrogen, methane, ethane, propane, carbon monoxide, carbon dioxide, mineralic oil (vapor and mist).

*Manufactured By:*

**Uniphos Envirotronic Pvt. Ltd**

P.O. Nahuli - 396 108

Tal. Umbergaon,

Dist: Valsad, Gujarat, India

Tel. : +91(260) 2730156 / 57 / 58

Fax : +91(260) 2730160

*Marketing Office:*

**Uniphos Envirotronic Pvt. Ltd**

Readymoney Terrace, 167,

Dr. Annie Besant Road, Worli,

Mumbai 400 018, India.

Tel. : +91(22) 6123 3500

Fax : +91(22) 2493 8826

+91 (22) 2497 8119